MIDMARK®

Installation Instructions

9A276001 (Non-Programmable) and 9A277001 (Programmable) Hand Control Kit

KIT COMPONENTS

Part Number	Description	Qty.
9A276001 or 9A277001	Hand Control	1
029-2272-00	Hand Control Mount Bracket Assy	1
040-0010-47	#10-24 x 3/8 Phillips Screw	2

REQUIRED TOOLS

#2 Phillips Screwdriver.

INTRODUCTION

This hand control accessory kit provides all the necessary components to mount and connect a 9A276001 or 9A277001 hand control to an appropriate examination table.

INSTALLATION

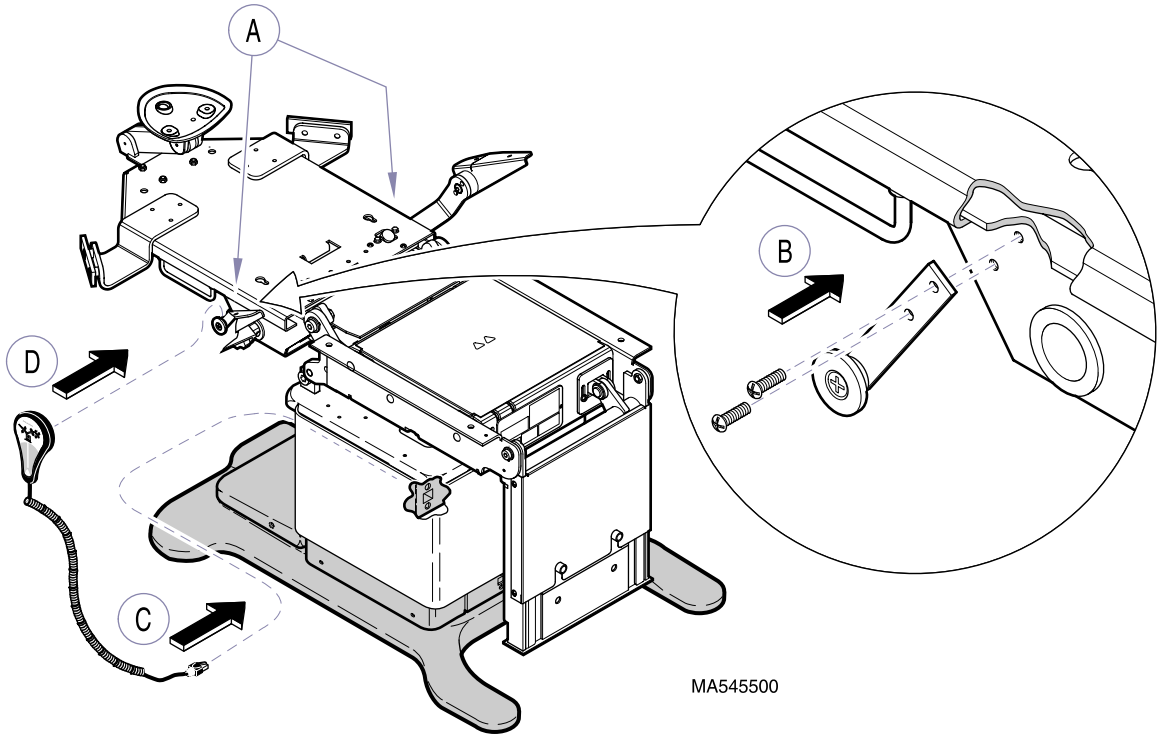

A. Determine which side of the table to install hand control mounting bracket; it may be installed on either side of table per doctor's preference.

B. Install hand control mount bracket assembly on back section of table with two phillips screws.

C. Insert the end of coil cord into hand control port (2) (If necessary, refer to the table's Installation & Operation Manual for instructions).

D. Hang the hand control on the hand control mount bracket; the hand control is now ready for use.

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

003-1057-00 Rev. A (12/99)

© Midmark Corporation - 1999